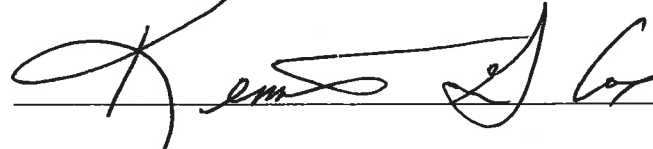


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N <u>130113</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>Kenneth G. Cox</u>	ID# <u>3527</u> Date <u>12/29/2011</u>
A Agency <u>Skagway Police Department</u> Phone # <u>(907) 983-2232</u>	
Instrument Location <u>Skagway Police Department 1st and State Street Skagway, AK 99840</u>	
B Alco S/N <u>X173019</u> Target Value <u>.082</u> High Pressure <u>500 psi</u>	
Alco Test Values <u>.079</u> <u>.080</u> 1st Alco 2nd Alco	
Signature <u></u>	
(OVER)	


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 1st day of Feb, 2012 UAK

 (Notary Seal Stamp)
Daniel L. Nicholas Nikki Roth
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130113

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130113

DECEMBER 29, 2011

OPERATOR'S NAME: *BMB 11/2/12*
COX/KENNETH/G
OPERATOR'S NUMBER: 3527
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
L

O.L. #: L
DEPT/AGENCY: SK61
CASE/REPORT: 2011-5303
TEST TYPE: U
ALCO TARGET VALUE: .002
ALCO S/N: X173019

— BREATH ANALYSIS —

.002 ADJUSTED FOR 29.55 in
ALCO TARGET .001 15:11
BLANK TEST .000 15:12
INTERNAL STANDARD VERIFIED 15:12
ALCO TV 29.55 in .079 15:13
BLANK TEST .000 15:13
SUBJECT SAMPLE *BMB 11/2/12* .000 15:14
BLANK TEST .000 15:15
ALCO TV 29.55 in .000 15:15
BLANK TEST .000 15:16

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130113

DECEMBER 29, 2011
TIME 15:07

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 29.55 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¡ ¢